



UV Talk Letter

Retrospective of Shimadzu UV-VIS Spectrophotometers— from Initial Release to Today

1. Introduction

UV-VIS spectrophotometers are the most commonly used analytical instrument using light. They are used in a wide variety of fields for applications such as quantitative analysis, colorimetry, measuring the thickness of thin films or coatings, or transmittance or reflectance measurements of optical elements.

2. First Shimadzu UV-VIS Spectrophotometer

Before the first UV-VIS spectrophotometer, quantitative analysis was performed using a colorimeter. However, in those days, a glass filter was used to output light of wavelengths corresponding to the sample color and that light was transmitted through containers containing a standard sample and unknown sample. Then the length of the container of (the optical path length of the light beam through) the standard sample (or alternatively the unknown sample) was visually adjusted with the naked eye, so that brightness of both beams was the same, where the concentration of the unknown sample was then determined based on the amount of adjustment. Therefore, there was significant potential for human error occurring in quantitated values. This situation was swept away in 1945, 70 years ago from now, when the world's first UV-VIS spectrophotometer was released in the United States. That UV-VIS spectrophotometer separated light into its different wavelengths using a prism, like the one illustrated in Fig. 1. The amount of light transmitted through the sample was measured using a photoelectric tube (a vacuum tube that uses the photoelectric effect to convert light energy into electrical energy). Due to its far superior performance than the colorimeter and dramatically higher precision and accuracy than other quantitative methods, the use of UV-VIS spectrophotometers quickly spread throughout the U.S. UV-VIS spectrophotometers were first imported to Japan immediately after their release in the U.S. Due to the significantly higher quantitative accuracy than the colorimeters commonly used at the time in Japan, the imported UV-VIS spectrophotometers caused a big sensation in the field of analytical chemistry, and Japanese-made UV-VIS spectrophotometers were eagerly waited at the same time. In response to this demand, engineers at Shimadzu used sketches of the U.S.-made UV-VIS spectrophotometer to start developing our own system based on trial and error. Soon they faced a major problem in the development process. The U.S.-made UV-VIS spectrophotometer used a hydrogen gas discharge tube as a light source for wavelengths below 400 nm,

Historically, it is one of the oldest analytical instruments as well. In the case of Shimadzu, we developed and released our first UV-VIS spectrophotometer using a prism in the early 1950s. This document reviews the history of Shimadzu UV-VIS spectrophotometers, from inception to today.

but no one in Japan manufactured hydrogen discharge tubes at the time. Consequently, they asked for help from a sister company in Kyoto city that was manufacturing mercury lamps. Shimadzu obtained the materials needed for manufacturing a hydrogen discharge tube and inspected prototypes, while the sister company designed and manufactured the tubes. With diligent effort by the sister company, we were finally able to create a hydrogen discharge tube that was equivalent to the U.S. product. The UV-VIS spectrophotometer imported from the U.S. used a photoelectric tube as a detector, but we received information about a photomultiplier tube developed in the U.S. that offered hundreds of times higher sensitivity than the photoelectric tube. Photomultiplier tubes are essentially a photoelectric tube with additional electric current amplification capability and are still used as detectors in UV-VIS spectrophotometers even today. Based on that information, we planned to create Japan's first photomultiplier tube to develop the world's first UV-VIS spectrophotometer equipped with a photomultiplier tube. To develop a Japanese photomultiplier tube, we asked a Japanese manufacturer of photoelectric tubes to jointly develop the tube with us. Thanks to the significant effort by that photoelectric tube manufacturer, we successfully created a photomultiplier tube that rivaled the performance of the U.S. product. In 1952, we completed Shimadzu's first UV-VIS spectrophotometer system, the QB-50 (Fig. 2). The system used a crystal prism as a spectroscopic element and was the first UV-VIS spectrophotometer in the world with a photomultiplier tube used as the detector. When the performance was compared to the U.S. UV-VIS spectrophotometer at a university in Kyoto city, the QB-50 was not inferior in performance to the U.S. system, but was also able to measure with adequate sensitivity 220 nm light that the American system could not. This system perfectly fit the needs of the times and sold well, becoming one of Shimadzu's leading products.

The prism was a triangular pole made of quartz or glass. The prism refracts the white light entering from the light source. The longer the wavelength of light is, the smaller the refractive index will be, and the shorter the wavelength, the larger the refractive index. Consequently, the light is divided into a spectrum of colors in order of wavelength - red, yellow, green, blue, and violet.

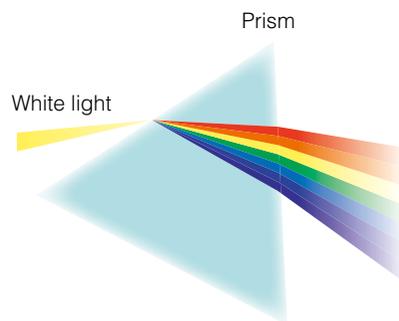


Fig. 1 Light Spectrum from a Prism



Fig. 2 Shimadzu QB-50 UV-Visible Spectrophotometer

3. Development History of Shimadzu UV-Vis Spectrophotometers

Since releasing the QB-50 UV-VIS spectrophotometer, Shimadzu has now developed and released over 70 new models of UV-VIS spectrophotometers so far, as listed in Table 1. Of those, several key models that formed the foundation of Shimadzu's reputation as a leader in manufacturing UV-VIS spectrophotometers are described below.

Table 1 History of Shimadzu UV-VIS Spectrophotometers

Year Released	Model
1952	QB-50
1956	QR-50
1957	RS-20
1958	RS-27
1961	SV-50
1963	QV-50, SG-15, SP-20
1964	MPS-50
1965	MPS-50L, AQV-50
1966	Double-40S/ 40SB/ 40D/ 40DB/ 40R/ 40DF
1968	Coloripet
1970	UV-200
1972	MPS-5000
1973	UV-210, SP-20A
1974	UV-300
1975	UV-140, UV-150
1976	UV-100, UV-110, UV-180, UV-190
1977	UV-220, UV-350, UV-360
1979	UV-365
1980	UV-120, UV-240
1981	UV-250, UV-3000
1982	MPS-2000

Year Released	Model
1983	UV-260
1985	UV-160
1986	UV-265
1987	UV-2100, UV-3100
1989	UV-2200, UV-3100PC
1990	UV-1200
1992	NIR-1500
1993	UV-1200V, UV-2100PC, UV-2200A
1994	UV-1600, UV-1600PC, UV-2400PC, UV-2500PC
1995	BioSpec-1600
1997	MultiSpec-1500, SP-20+
1998	Uvmini-1240, MPS-2400
1999	UV-1650, UV-2450, UV-2550
2000	UV-3150
2001	UV-1700
2004	UV-3600, SolidSpec-3700/3700DUV
2006	BioSpec-mini, MPS-2450
2007	UV-1800
2008	BioSpec-nano
2011	UV-2600, UV-2700
2014	UV-3600 Plus, UV-1280

3-1. History of Double-Beam Spectrophotometers

A system that continuously scans samples with different monochromator wavelengths and automatically records the resulting spectrum on a data recorder is referred to as a recording spectrophotometer. Recording spectrophotometers use a double-beam configuration, where monochromatic light is split into two light beams, a sample light beam and reference light beam, which are alternately transmitted through the sample compartment for measurement. In contrast, the QB-50 used a single-beam configuration, where only one beam was transmitted through the sample compartment. Double-beam recording spectrophotometers were also first developed in the U.S. and imported into Japan. Due to the ability to measure spectra, demand increased for double-beam spectrophotometers, which resulted in releasing the RS-20 in 1957, shown in Fig. 3. The RS-20 monochromator featured a double-beam optical system installed in the same shape housing as the QB-50. The RS-20 represents the starting point for Shimadzu's current line of double-beam spectrophotometers, which is now one of the main product lines at Shimadzu.

In the 1970s, the UV-200 shown in Fig. 4 was released as a smaller and more economical model. The UV-200 features a double-beam optical system with symmetric sample and reference light beams that have identical optical path lengths and an identical number of mirrors reflecting the beams, as shown in Fig 5. Consequently, it offered outstanding baseline flatness, transmittance accuracy, and temporal stability. This configuration is still used today.

In 1980, the UV-240 was released with separate control and

measurement units, as shown in Fig. 6. That innovative model was acclaimed for being the first UV-VIS spectrophotometer system available with the operator interface separated from the measurement unit. The control unit featured a graphic recorder that could print spectra, measurement conditions, quantitative analysis calculation results, and so on, on chart paper. It also featured a holographic grating as the device used to disperse light. Holographic gratings are diffraction gratings made by using laser holographic interference fringes to form parallel grooves and then using an ion beam to etch the grooves. Compared to conventional mechanically machined diffraction gratings, holographic gratings provide superior diffraction efficiency and lower stray light levels. The UV-240 was one of our best sellers at the time, with over 3600 units sold worldwide. Around 1990, the cost of personal computers had decreased sufficiently and the demand increased for computer-controlled UV-VIS spectrophotometers. Consequently, we released the UV-2100PC in 1993 and the UV-2400PC and UV-2500PC models in 1994. Currently, we are selling the successors to those models, the UV-2600 and UV-2700.

In 1985, we released the UV-160, shown in Fig. 7, which was an all-in-one double-beam spectrophotometer that included a CRT screen, keypad, printer, and other functionality all integrated in a single unit. Due to its low price and high performance, we sold over 20,000 units worldwide, which contributed significantly to the widespread use of UV-VIS spectrophotometers. The UV-1800 currently being sold features a similar configuration to that system.



Fig. 3 Shimadzu RS-20 UV-VIS Spectrophotometer

(Excerpted from p. 275 of 'Shimadzu Analytical Instruments 'People & Stories' from Pioneers to Leaders in 60 Years' planned & compiled by Hideki Makabe, Published by Shimadzu Corporation, 2006)



Fig. 4 Shimadzu UV-200 UV-VIS Spectrophotometer

(Excerpted from p. 289 of 'Shimadzu Analytical Instruments 'People & Stories' from Pioneers to Leaders in 60 Years' planned & compiled by Hideki Makabe, Published by Shimadzu Corporation, 2006)

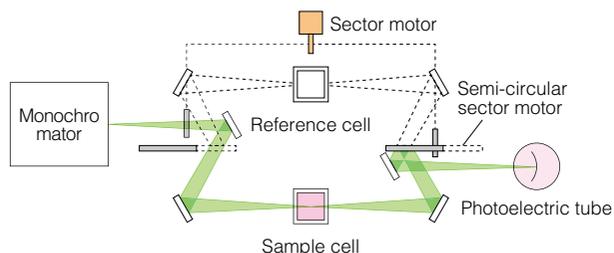


Fig. 5 Optical System in Symmetric Double-Beam Spectrophotometer

(Excerpted from p. 289 of 'Shimadzu Analytical Instruments 'People & Stories' from Pioneers to Leaders in 60 Years' planned & compiled by Hideki Makabe, Published by Shimadzu Corporation, 2006)



Fig. 6 Shimadzu UV-240 UV-VIS Spectrophotometer



Fig. 7 Shimadzu UV-160 UV-VIS Spectrophotometer

3-2. History of Double-Monochromator and UV-VIS-NIR Spectrophotometers

Double-monochromator spectrophotometers reduce stray light by monochromating the light from the light source in two consecutive stages. Shimadzu's first double-monochromator spectrophotometer was the Double-40 series, released in 1966. Double-40 series double-monochromator spectrophotometers included both a prism and diffraction grating and were available in either single-beam or double-beam configuration. In 1981, Shimadzu released the UV-250, the double-monochromator version of the UV-240 mentioned above. UV-2500PC, UV-2550PC, and UV-2700 models, mentioned above, were also released as part of the same series. The UV-2700 model currently being sold, features a diffraction grating that achieves ultra low stray light levels, which expands the measurement range to 8 Abs and accurately determines transmittances to 0.000001 % (1 part in 100 million). Spectrophotometers capable of measuring light in the ultraviolet, visible, and near infrared regions are called UV-VIS-NIR spectrophotometers. In 1958, the RS-27 was released as a version

of the RS-20 mentioned above with an extended measurement range that includes the near infrared region. It was Shimadzu's first UV-VIS-NIR spectrophotometer. The RS-27 was a single-monochromator design with a prism-based monochromator. In 1977, Shimadzu released the UV-360, Shimadzu's first double-monochromator UV-VIS-NIR spectrophotometer, which was equipped with both prism and diffraction grating-based monochromators. Its successor model, the UV-365, was released in 1979, shown in Fig 8. It was the first UV-VIS(-NIR) spectrophotometer equipped with a microprocessor, which were gaining widespread popularity at the time. The UV-3600 Plus and SolidSpec-3700 models, which feature three detectors (a photomultiplier tube, InGaAs detector, and cooled PbS detector) and higher sensitivity in all measurement wavelength regions, are currently Shimadzu's top-of-the-line UV-VIS spectrophotometer models that have both flowed from the original RS-27 model.



Fig. 8 Shimadzu UV-365 UV-VIS-NIR Spectrophotometer

4. Unique UV-VIS Spectrophotometers

Around 1960, a university in Tokyo asked Shimadzu to develop a UV-VIS spectrophotometer capable of measuring spectra from semi-transparent samples with turbidity. That resulted in developing a unique unprecedented instrument. To increase the detection efficiency of scattered light emitted from the samples, the instrument used an end-on photomultiplier tube detector with a light-receiving surface on the measuring head, as shown in Fig. 9. Due to its ability to measure transparent, semi-transparent, or opaque samples (reflectance was measured for opaque samples), the instrument was released in 1964 with the model name MPS-50 (based on an acronym for "multipurpose system"). It caused a major response from academic institutions and companies involved in biochemistry. The MPS-50 still used vacuum tubes, but transistors and integrated circuit devices were used for the MPS-5000 successor model (Fig. 10) released in 1972, which was smaller and offered higher performance.



Fig. 9 End-On Photomultiplier Tube

(Excerpted from p. 282 of "Shimadzu Analytical Instruments 'People & Stories' from Pioneers to Leaders in 60 Years" planned & compiled by Hideki Makabe, Published by Shimadzu Corporation, 2006)

Another unique UV-VIS spectrophotometer model was the UV-300 released in 1974. Referred to as a dual-wavelength double-beam recording spectrophotometer, the UV-300 featured two built-in monochromators connected in parallel, which allowed using one monochromator to measure the absorbance spectrum, as usual, while the other measured absorbance at a specific fixed wavelength, so that the difference in absorbance measured at the two wavelengths could be recorded as a spectrum. That allowed measurement of spectra without being affected by turbidity. In 1981, a successor model was released, the UV-3000 shown in Fig. 11, which featured improved functionality using a microprocessor and a measurement wavelength range from 190 nm to 900 nm. Both the MPS series and UV-300 series were unique UV-VIS spectrophotometers, but sales were discontinued after demand decreased.

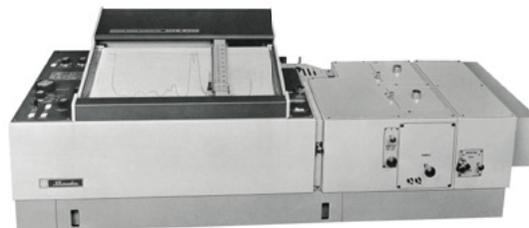


Fig. 10 Shimadzu MPS-5000 Multipurpose Recording Spectrophotometer



Fig. 11 Shimadzu UV-3000 Dual-Wavelength Double-Beam Recording Spectrophotometer

5. Summary

Shimadzu has sold about 190,000 UV-VIS spectrophotometers around the world, starting with the QB-50 released in 1952. Today, UV-VIS spectrophotometers have become an essential analytical instrument for quantitative analysis or for determining the optical properties of substances. Consequently, Shimadzu will continue to offer improved systems that better meet the needs of various users.

This article was based on "Shimadzu Analytical Instruments 'People & Stories' from Pioneers to Leaders in 60 Years," planned and compiled by Hideki Makabe, published by Shimadzu Corporation in 2006.